


KINGSCLIFF EDM BASELINE

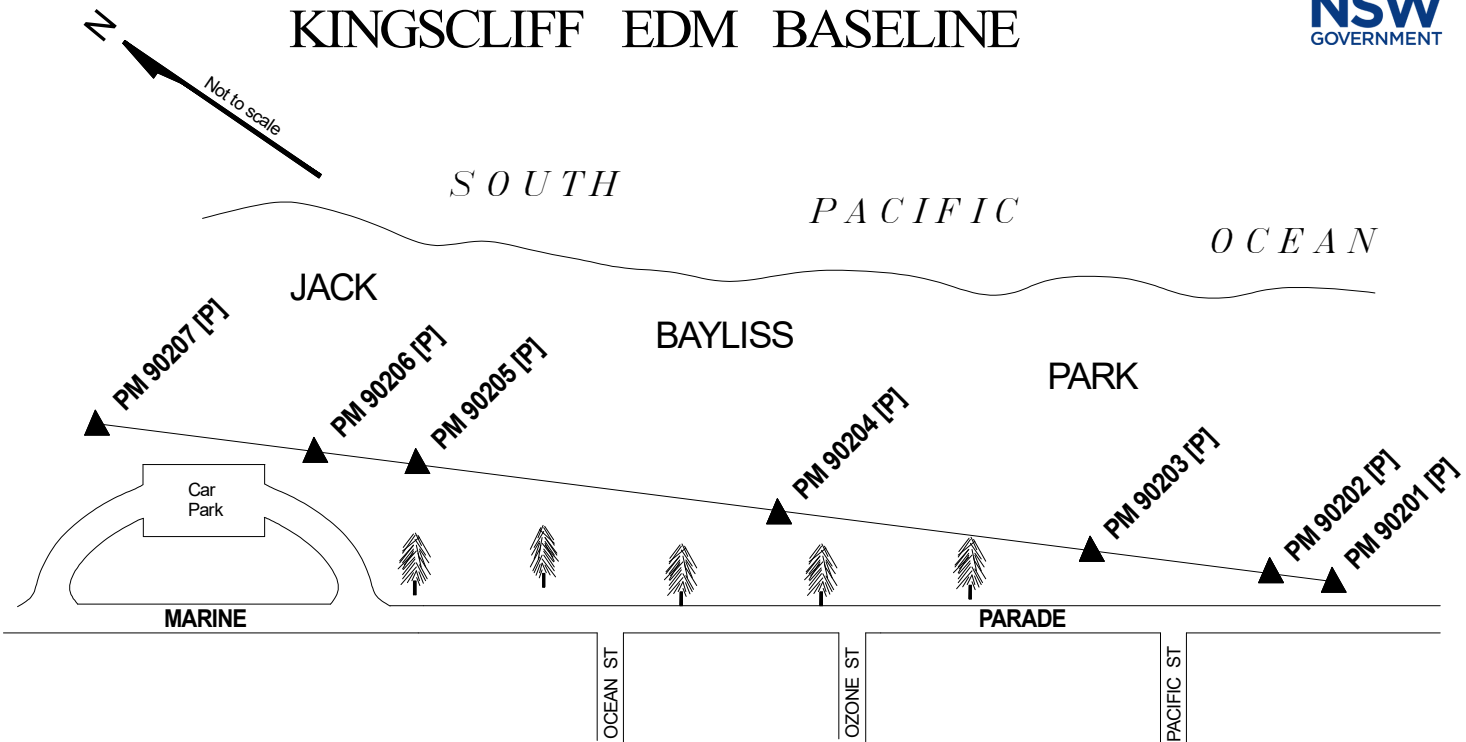

ACCESS : Authorised access only - For baseline booking please refer to website: www.six.nsw.gov.au/edmbooking (3/8" Allen key required to remove pillar caps)

HORIZONTAL DISTANCES (metres) AT DATUM 7.443 m AHD

From	To	Distance	Mark	R.L. (AHD) *
PM 90201	PM 90202	28.3295	PM 90201	9.388
PM 90201	PM 90203	130.8332	PM 90202	9.012
PM 90201	PM 90204	332.6291	PM 90203	8.258
PM 90201	PM 90205	564.2211	PM 90204	7.443
PM 90201	PM 90206	628.3345	PM 90205	7.904
PM 90201	PM 90207	721.2590	PM 90206	8.114
			PM 90207	8.646

* The Reduced Levels (in metres AHD) were re-verified at this date.

Method of verification: VA-QM-01 and NMI's Verifying Authorities Handbook, 2nd Ed. November 1988

Distances by the Surveyor-General of NSW, in accordance with the verification of a Reference standard of length as prescribed by the National Measurement Act 1960.

Instrument used : Leica TS 30, Serial No. 360783

Verified in accordance with Regulation 13 of the National Measurement Regulations 1999.

Uncertainty of distances: $\pm (0.5 + 1.3 \times 10^{-3}L)$ mm, L= length in metres

This uncertainty is calculated in accordance with the principles of the ISO Guide to the Expression of Uncertainty in Measurement, with an interval estimated to have a confidence level of 95% and a coverage factor of 2. The uncertainty applies at the time of measurement only and takes no account of pillar movement that may occur after the date of verification.



Accredited for compliance with ISO/IEC 17025 - Calibration.
The results of the tests, calibrations and/or measurements included in this document are traceable to Australian national standards.
This document shall not be reproduced, except in full.

NATA Accredited Laboratory Number: 14965

R K Lock date: 27/04/22
Senior Surveyor
(Legal Metrology Officer)
for the Surveyor-General of NSW
Date of Verification: 06 April 2022