


# WOLLONGONG EDM TESTLINE

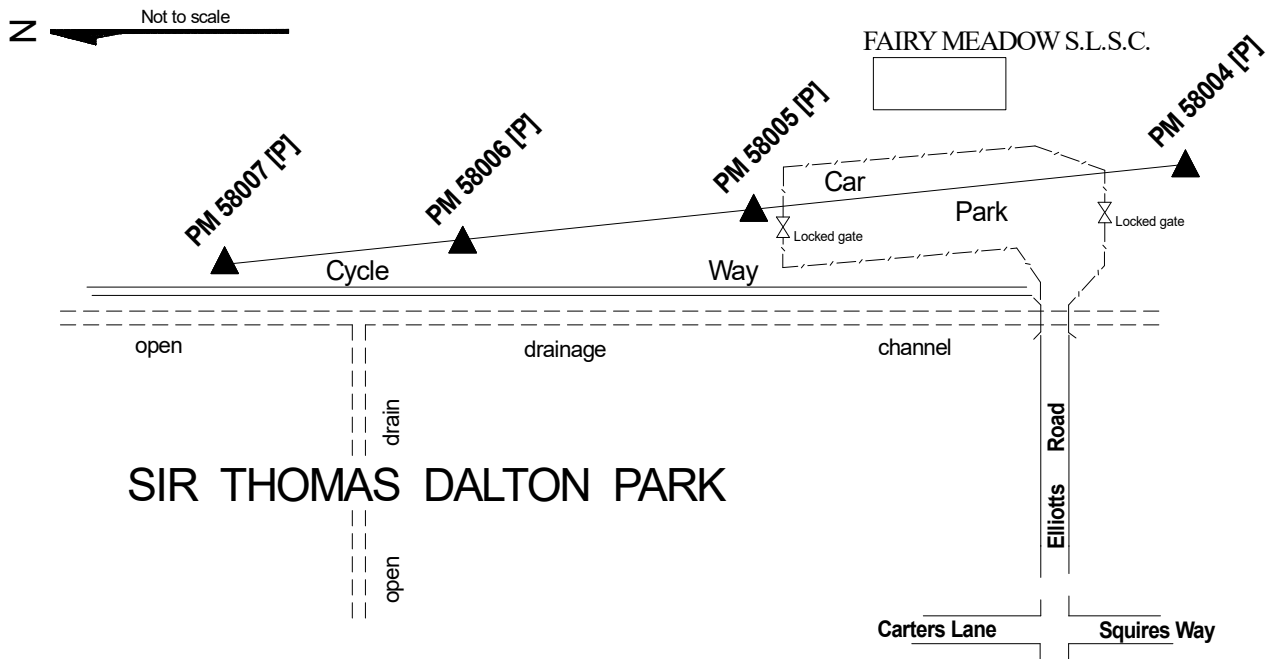

ACCESS : Authorised access only - For baseline booking & to obtain security code to padlock: [www.six.nsw.gov.au/edmbooking](http://www.six.nsw.gov.au/edmbooking) (10mm Allen key required to remove pillar caps.)

HORIZONTAL DISTANCES (metres) AT DATUM 5.942 m AHD

From	To	Distance	Mark	RL (AHD) *
PM 58004	PM 58005	194.9675	PM 58004	7.425
PM 58004	PM 58006	417.4720	PM 58005	6.423
PM 58004	PM 58007	599.9682	PM 58006	5.942
			PM 58007	6.724

\* The Reduced Levels (in metres AHD) were re-verified at this date.

Method of verification: VA-QM-01 and NMI's Verifying Authorities Handbook, 2nd Ed. November 1988

Distances by the Surveyor-General of NSW, in accordance with the verification of a Reference standard of length as prescribed by the National Measurement Act 1960.

Instrument used : Leica TS 30, Serial No. 360783

Verified in accordance with Regulation 13 of the National Measurement Regulations 1999.

Uncertainty of distances:  $\pm (0.5 + 1.3 \times 10^{-3}L)$  mm, L= length in metres

This uncertainty is calculated in accordance with the principles of the ISO Guide to the Expression of Uncertainty in Measurement, with an interval estimated to have a confidence level of 95% and a coverage factor of 2. The uncertainty applies at the time of measurement only and takes no account of pillar movement that may occur after the date of verification.



Accredited for compliance with ISO/IEC 17025 - Calibration  
 The results of the tests, calibrations and/or measurements included in this document are traceable to Australian national standards.  
 This document shall not be reproduced, except in full.  
 NATA Accredited Laboratory Number: 14965

R. K. Lock date: 30/11/21  
 Senior Surveyor  
 (Legal Metrology Officer)  
 for the Surveyor-General of NSW

Date of Verification: 15 November 2021