



WAGGA WAGGA EDM TESTLINE

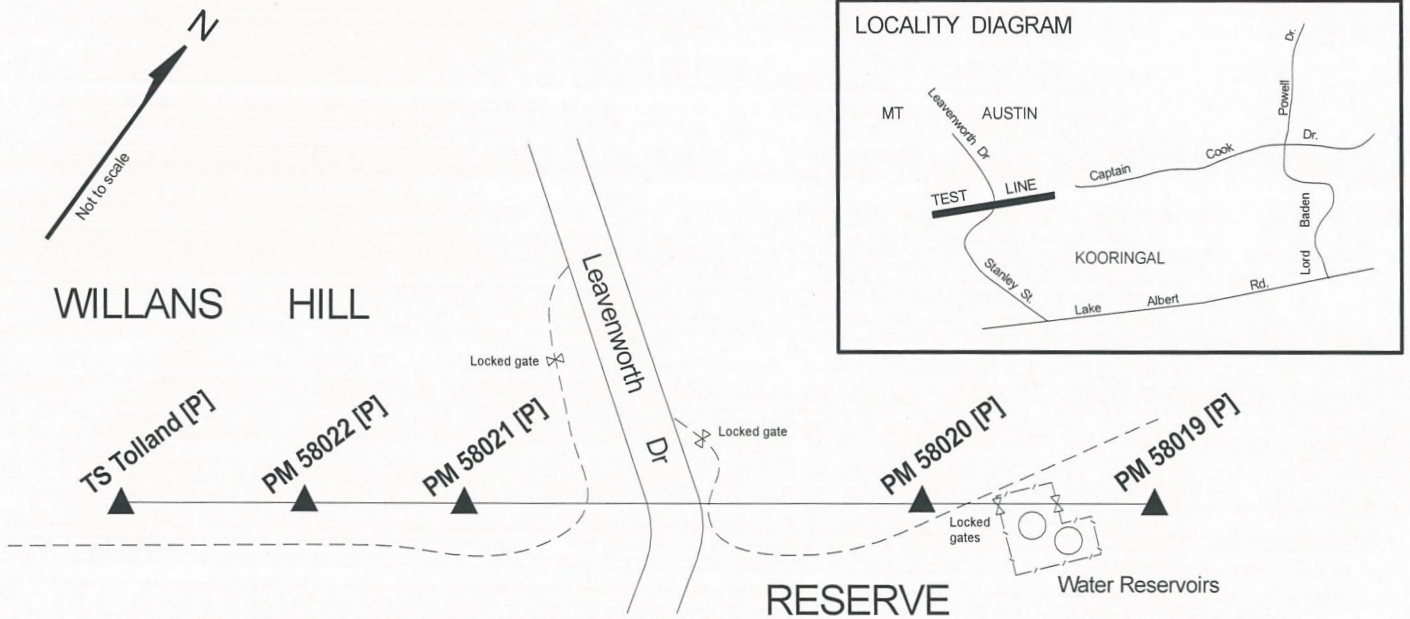

ACCESS : Authorised access only. Obtain keys to Reserve & water reservoir compound from DPI - Lands, cnr Johnston & Tarcutta Sts (office hrs 0900 -1200) ph: 6937 2700. Baseline Booking: [www.six.nsw.gov.au/edmbooking](http://www.six.nsw.gov.au/edmbooking) (3/8" Allen key required to remove pillar caps)

HORIZONTAL DISTANCES AT DATUM 289.600 m AHD

From	To	Distance	Mark	R.L. (AHD) *
PM 58019	PM 58020	138.6003	PM 58019	306.520
PM 58019	PM 58021	404.5795	PM 58020	299.433
PM 58019	PM 58022	459.9768	PM 58021	289.600
PM 58019	TS TOLLAND	534.9560	PM 58022	298.569
			TS TOLLAND	308.331

\* The Reduced Levels (in metres AHD) were not re-verified at this date.

Method of verification: VA-QM-01 and NMI's Verifying Authorities Handbook, 2nd Ed. November 1988

Distances by the Surveyor-General of NSW, in accordance with the verification of a Reference standard of length as prescribed by the National Measurement Act 1960.

Instrument used : Leica TS 30, Serial No. 360783

Verified in accordance with Regulation 13 of the National Measurement Regulations 1999.


Uncertainty of distances: +/- (0.6 + 1.3 x 10<sup>-3</sup>L) mm, L= length in metres

This uncertainty is calculated in accordance with the principles of the ISO Guide to the Expression of Uncertainty in Measurement, with an interval estimated to have a confidence level of 95% and a coverage factor of 2. The uncertainty applies at the time of measurement only and takes no account of pillar movement that may occur after the date of verification.



Accredited for compliance with ISO/IEC 17025 - Calibration  
The results of the tests, calibrations and/or measurements included in this document are traceable to Australian national standards.  
This document shall not be reproduced, except in full.

NATA Accredited Laboratory Number: 14965

  
R. K. Lock date 17/10/19  
Senior Surveyor  
(Legal Metrology Officer)  
for the Surveyor-General of NSW

Date of Verification: 6 August 2019