


WAGGA WAGGA EDM TESTLINE

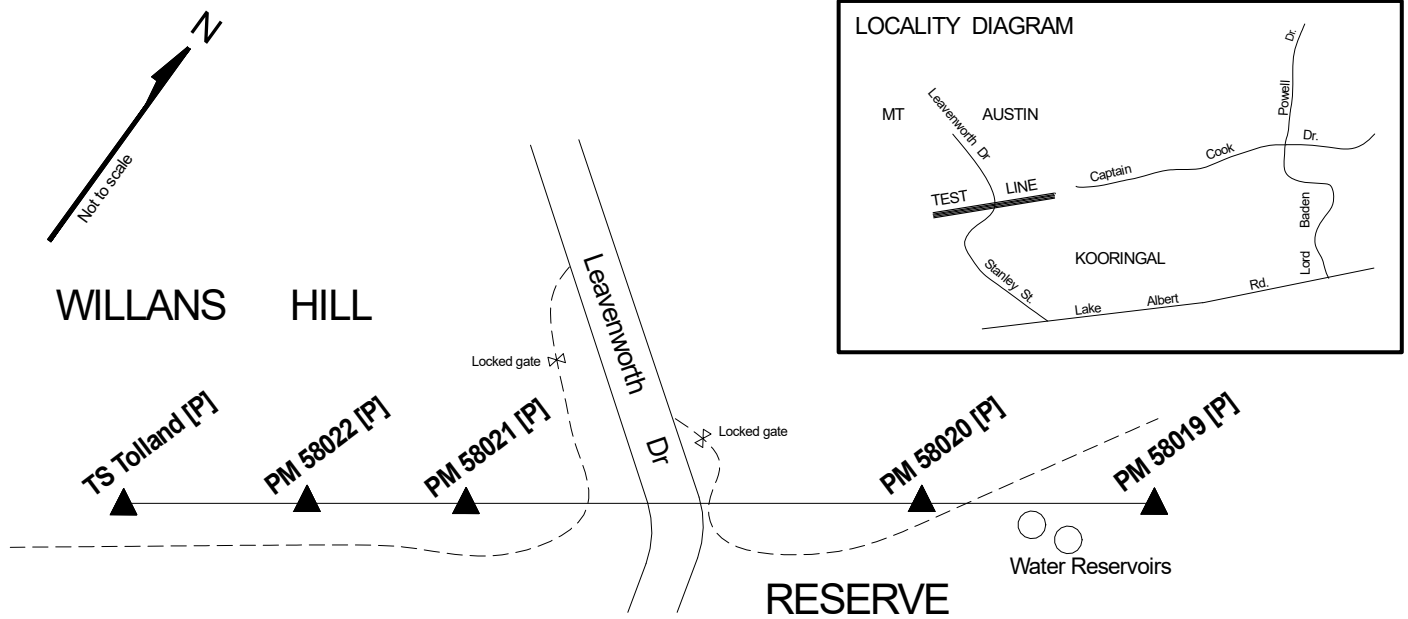

Authorised Access Only - For baseline booking & to obtain security code to padlock: www.spatial.nsw.gov.au/edmbooking (3/8" Allen key required to remove pillar caps)

HORIZONTAL DISTANCES (metres) at datum 289.600 m AHD

From	To	Distance	Mark	R.L. (AHD) *
PM 58019	PM 58020	138.6000	PM 58019	306.516
PM 58019	PM 58021	404.5793	PM 58020	299.431
PM 58019	PM 58022	459.9762	PM 58021	289.600
PM 58019	TS TOLLAND	534.9548	PM 58022	298.567
			TS TOLLAND	308.330

* The Reduced Levels (metres) were determined at this date and are on an approximate AHD datum. These height measurements are outside the NATA Scope of Accreditation.

Method of verification: Surveyor-General procedure VA-QMS-01

Reference instrument used : Leica TS 30, Serial No. 360783
Verified in accordance with Regulation 13 of the National Measurement Regulations 1999.

Uncertainty of distances: $\pm (0.5 + 1.3 \times 10^{-3}L)$ mm, L= length in metres
This uncertainty is calculated in accordance with the principles of the ISO Guide to the Expression of Uncertainty in Measurement, with an interval estimated to have a confidence level of 95% and a coverage factor of 2. The uncertainty applies at the time of measurement only and takes no account of pillar movement that may occur after the date of verification.



Accredited for compliance with ISO/IEC 17025 - Calibration
All equipment used is calibrated by NATA accredited laboratories, and the measurements included in this document are traceable to SI units. This document shall not be reproduced, except in full.

NATA Accredited Laboratory Number: 14965