


## BANKSTOWN EDM TESTLINE

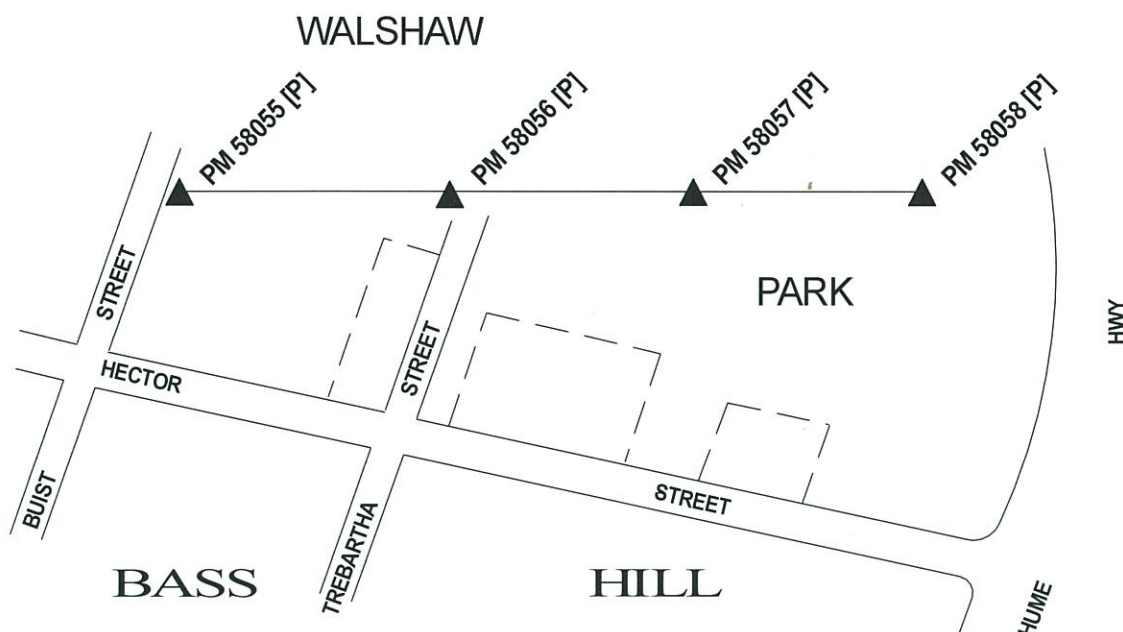

ACCESS : Authorised access only - For baseline booking please refer to website: [www.six.nsw.gov.au/edmbooking](http://www.six.nsw.gov.au/edmbooking)  
(10mm Allen key required to remove pillar caps)

HORIZONTAL DISTANCES (metres) AT DATUM 47.484 m AHD

From	To	Distance	Mark	RL (AHD) *
PM 58055	PM 58056	202.0791	PM 58055	47.484
PM 58055	PM 58057	458.7422	PM 58056	48.445
PM 58055	PM 58058	605.0061	PM 58057	50.739
			PM 58058	57.634

\* The Reduced Levels (in metres AHD) were not re-verified at this date.

Method of verification: VA-QM-01 and NMI's Verifying Authorities Handbook, 2nd Ed. November 1988

Distances by the Surveyor-General of NSW, in accordance with the verification of a Reference standard of length as prescribed by the National Measurement Act 1960.

Instrument used : Leica TS 30, Serial No. 360783

Verified in accordance with Regulation 13 of the National Measurement Regulations 1999

Uncertainty of distances:  $\pm (0.7 + 1.3 \times 10^{-3} L)$  mm, L= length in metres

This uncertainty is calculated in accordance with the principles of the ISO Guide to the Expression of Uncertainty in Measurement, with an interval estimated to have a confidence level of 95% and a coverage factor of 2. The uncertainty applies at the time of measurement only and takes no account of pillar movement that may occur after the date of verification.



Accredited for compliance with ISO/IEC 17025 - Calibration

The results of the tests, calibrations and/or measurements included in this document are traceable to Australian national standards.

This document shall not be reproduced, except in full.

NATA Accredited Laboratory Number: 14965



R. K. Lock date 4/10/18

Senior Surveyor  
(Legal Metrology Officer)  
for the Surveyor-General of NSW

Date of Verification: 25 Sep 2018